

CARRYING CASE



MID LEG STRAP



TRACTION CORD



ANKLE STRAP

DISTAL CLAMP

PROXIMAL CLAMP

END CAP

GROIN STRAP

MALE BUCKLE

FEMALE BUCKLE

Any serious incident that has occurred in relation to this device should be reported to Tri-Tech Forensics and to the Competent Authority of the Member State in which the user and/or patient is established.

MD	Medical Device	UDI	Unique Device Identifier	EC REP	Authorized European Representative	SN	Serial Number		Date of Manufacture
	Not Made with Natural Rubber Latex		Manufacturer		Consult Instructions For Use	LOT	Lot Number		

U.S. Patents: 6,394,972 - 6,786,882 - 6,913,587
 Meets MIL-STD-810G, 501.5
 EP Pat. (DE, FR, UK) No. 3226817
 Canadian Patent 3007222

Intended Purpose:
 The Slishman Traction Splint is intended for use by healthcare professionals for the stabilization and traction of fractured femurs. The device can also be used as a simple splint for any extremity fracture, strain, or sprain.

Contraindications and Warnings:
 Traction should not be used for hip, pelvis or humerus fractures, unless a test pull of the traction cord provides immediate pain relief or return of perfusion. Also, traction should be avoided for grossly open and contaminated fractures. If the splint comes in contact with toxins like organophosphates, radioactive material, or excessive bodily fluids, then it should be disposed of as deemed appropriate for hazardous materials or biological wastes. If it can be washed and sanitized, then reuse is acceptable.

Cleaning and Disposal:
 The Slishman Traction Splint should be thoroughly cleaned by washing with warm water and disinfectant and then wiped down with a clean rag. If the entire device is contaminated, place it in a red biohazard bag and dispose according to your hazardous waste protocol. Contaminated hip/groin strap can be removed from the device and laundered in the washing machine with detergent and disinfectant added. Do not use bleach. Remove the strap and hang to dry. Do not put straps in dryer. The outer tube strap is neoprene and should not be cleaned using hot water. Instead, wipe the strap thoroughly using disinfecting wipes. The straps should be considered disposable if they are grossly contaminated or if cleaning requires exuberant effort. These items should be replaced rather than cleaned.

Tri-Tech Forensics, Inc. dba Rescue Essentials
 3811 International Blvd NE, Ste 100
 Leland, NC 28451 USA

REF #10-0262 NSN: 6515-01-631-3182
 NATO: 6515-32-083-5266

CE **EC REP** **RESCUE ESSENTIALS**
 MedEnvoy Global B.V.
 Prinses Margrietplantsoen 33,
 Suite 123 2595AM The Hague
 The Netherlands

North Carolina USA • 910-830-0286
 www.rescue-essentials.com


SLISHMAN TRACTION SPLINT



DIRECTIONS FOR USE

Slushman Traction Splint (STS)

INSTRUCTIONS FOR USE

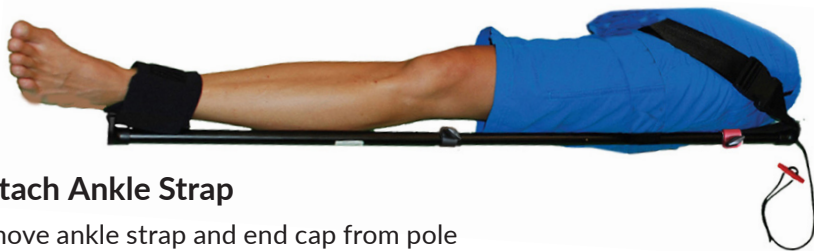

Prior to application assess CMS (circulation, motor and sensory) function and pain level per local protocol.

1. Attach Ankle Strap

- Remove ankle strap and end cap from pole
- Unroll ankle strap and apply with end cap lateral and facing up to receive splint pole
- Secure with hook and loop wrap



NOTE: May apply ankle strap above calf in cases of lower leg injury.




2. Attach Groin Strap

- Rest female buckle on anterior thigh
- Wrap male buckle and strap behind thigh
- Snap male to female buckle and tighten



3. Apply Coarse Traction

- Extend distal pole after releasing thumb screw on black pole clamp
- Insert distal pole into ankle strap end cap
- After achieving desired length, tighten thumb screw

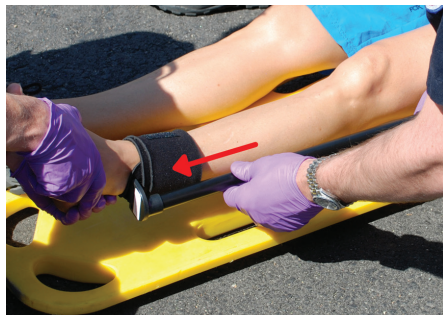

4. Apply Fine Traction

- Release thumb screw on red pole clamp
- Pull cord to apply desired traction
- Tighten thumb screw on red pole clamp and release cord



5. Reassess and Monitor

- Reassess CMS and pain level
- Adjust traction as needed to minimize pain, while maintaining perfusion
- For rotational stability attach mid leg strap to splint and wrap (one or both legs) below knee



NOTE: IF CLAMP SLIDES OFF POLE

In the event the red or black pole clamp slides off the pole, simply loosen the thumb screw and push the pole clamp back over the end of the pole and align where indicated. Tighten thumb screw to secure in place.



PEDIATRIC APPLICATION

For patients under 110 cm (approx. 43 inches) in height and/or 3 years or less in age, lengthen the groin strap allowing the splint to rest more proximal to the hip.



SCAN ME